



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification ⁶ : A61B 5/00</p>	A2	<p>(11) International Publication Number: WO 99/22640</p> <p>(43) International Publication Date: 14 May 1999 (14.05.99)</p>								
<table style="width: 100%; border: none;"> <tr> <td style="width: 50%; vertical-align: top; padding: 5px;"> <p>(21) International Application Number: PCT/US98/22961</p> <p>(22) International Filing Date: 30 October 1998 (30.10.98)</p> <p>(30) Priority Data:</p> <table style="width: 100%; border: none;"> <tr> <td style="width: 33%;">08/961,294</td> <td style="width: 33%;">30 October 1997 (30.10.97)</td> <td style="width: 33%;">US</td> </tr> <tr> <td>60/093,041</td> <td>10 November 1997 (10.11.97)</td> <td>US</td> </tr> </table> <p>(71) Applicant: HYPERMED IMAGING, INC. [US/US]; 315 Russett Avenue, Chestnut Hill, MA 02115 (US).</p> <p>(72) Inventors: LEWIS, Edgar, N.; 18420 Shady View Lane, Brookeville, MD 20833 (US). FREEMAN, Jenny, E.; 27 Lyon Road, Chestnut Hill, MA 02167 (US).</p> <p>(74) Agents: REMENICK, James et al.; Baker & Botts, L.L.P., The Warner, Suite 1300, 1299 Pennsylvania Avenue, N.W., Washington, DC 20004-2400 (US).</p> </td> <td style="width: 50%; vertical-align: top; padding: 5px;"> <p>(81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, HR, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).</p> <p>Published <i>Without international search report and to be republished upon receipt of that report.</i></p> </td> </tr> </table>			<p>(21) International Application Number: PCT/US98/22961</p> <p>(22) International Filing Date: 30 October 1998 (30.10.98)</p> <p>(30) Priority Data:</p> <table style="width: 100%; border: none;"> <tr> <td style="width: 33%;">08/961,294</td> <td style="width: 33%;">30 October 1997 (30.10.97)</td> <td style="width: 33%;">US</td> </tr> <tr> <td>60/093,041</td> <td>10 November 1997 (10.11.97)</td> <td>US</td> </tr> </table> <p>(71) Applicant: HYPERMED IMAGING, INC. [US/US]; 315 Russett Avenue, Chestnut Hill, MA 02115 (US).</p> <p>(72) Inventors: LEWIS, Edgar, N.; 18420 Shady View Lane, Brookeville, MD 20833 (US). FREEMAN, Jenny, E.; 27 Lyon Road, Chestnut Hill, MA 02167 (US).</p> <p>(74) Agents: REMENICK, James et al.; Baker & Botts, L.L.P., The Warner, Suite 1300, 1299 Pennsylvania Avenue, N.W., Washington, DC 20004-2400 (US).</p>	08/961,294	30 October 1997 (30.10.97)	US	60/093,041	10 November 1997 (10.11.97)	US	<p>(81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, HR, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).</p> <p>Published <i>Without international search report and to be republished upon receipt of that report.</i></p>
<p>(21) International Application Number: PCT/US98/22961</p> <p>(22) International Filing Date: 30 October 1998 (30.10.98)</p> <p>(30) Priority Data:</p> <table style="width: 100%; border: none;"> <tr> <td style="width: 33%;">08/961,294</td> <td style="width: 33%;">30 October 1997 (30.10.97)</td> <td style="width: 33%;">US</td> </tr> <tr> <td>60/093,041</td> <td>10 November 1997 (10.11.97)</td> <td>US</td> </tr> </table> <p>(71) Applicant: HYPERMED IMAGING, INC. [US/US]; 315 Russett Avenue, Chestnut Hill, MA 02115 (US).</p> <p>(72) Inventors: LEWIS, Edgar, N.; 18420 Shady View Lane, Brookeville, MD 20833 (US). FREEMAN, Jenny, E.; 27 Lyon Road, Chestnut Hill, MA 02167 (US).</p> <p>(74) Agents: REMENICK, James et al.; Baker & Botts, L.L.P., The Warner, Suite 1300, 1299 Pennsylvania Avenue, N.W., Washington, DC 20004-2400 (US).</p>	08/961,294	30 October 1997 (30.10.97)	US	60/093,041	10 November 1997 (10.11.97)	US	<p>(81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, HR, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).</p> <p>Published <i>Without international search report and to be republished upon receipt of that report.</i></p>			
08/961,294	30 October 1997 (30.10.97)	US								
60/093,041	10 November 1997 (10.11.97)	US								
<p>(54) Title: MULTISPECTRAL/HYPERSPECTRAL MEDICAL INSTRUMENT</p> <div style="text-align: center; padding: 20px;"> </div>										
<p>(57) Abstract</p> <p>A medical instrument that comprises: a first-stage optic responsive to a tissue surface of a patient; a spectral separator optically responsive to the first stage optic and having a control input; an imaging sensor optically responsive to the spectral separator and having an image data output; and a diagnostic processor having an image acquisition interface with an input responsive to the imaging sensor and a filter control interface having a control output provided to the control input of the spectral separator.</p>										

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

MULTISPECTRAL/HYPERSPECTRAL MEDICAL INSTRUMENT

Field of the Invention

The invention relates to a surgical and diagnostic instrument for performing real-time general-purpose imaging during surgery, clinical procedures, or other medical evaluations.

Background of the Invention

Spectroscopic imaging devices which employ Acousto-Optic Tunable Filters (AOTF), Liquid Crystal Tunable Filters (LCTF), or dispersive gratings are known. Such devices have been used for microscopy and remote sensing.

Summary of the Invention

Generally, the invention features a medical instrument that includes an optic responsive to a surface of tissue of a patient, a spectral separator optically responsive to the optic, and an imaging sensor optically responsive to the spectral separator. The instrument also includes a diagnostic processor having an image acquisition interface responsive to the imaging sensor and a filter control interface to which the spectral separator is responsive.

The spectral separator can be a tunable filter, such as a liquid crystal tunable filter, and the imaging sensor can be a two-dimensional imaging array, such as a charge coupled device. The optic can include a macro lens, an adjustable lens, or a probe that includes an imaging fiber optic cable, and a stand can be connected relative to the optic to position the optic relative to the patient. The control interface can be operable to adjust the filter at least twenty times to acquire hyperspectral data for redisplay in real time. The medical instrument can perform diagnostic processing for images acquired exclusively under visible light.

The diagnostic processor can also include a general-purpose processing module and diagnostic protocol modules, which can each include filter transfer functions and an image processing protocol. The general-purpose processing module can be operative to instruct the

filter to successively apply the filter transfer functions to light collected from the patient, to acquire from the imaging sensor a number of images of the collected light each obtained after one of the filter transfer functions is applied, and to process the acquired images according to the image processing protocol to obtain a processed display image. The general-purpose processor can be a real-time processor operative to generate a processed display image within a time period on the order of the persistence of human vision. It may also be operative to acquire some images more slowly depending on the number of wavelengths and complexity of diagnostic processing protocol. The sensor and filter can be operative in the visible, infra-red, and UV regions.

Instruments according to the invention are advantageous in that they can permit a surgeon or a physician to diagnose a medical condition or develop a surgical strategy based on real-time images obtained during surgery or in the course of performing clinical procedures or other medical evaluations. The physician may therefore be able to obtain significantly more information about a patient's condition than he might otherwise have been able to assemble by presenting an interactive interface. This additional information may permit a given surgical procedure to be carried out more precisely and may lead to more successful surgical results. It may also enhance the precision and results of other types of medical evaluations and procedures.

The general-purpose nature of the instrument can also help the surgeon develop significant amounts of medical information in time-critical surgical situations. For example, a patient may undergo relatively straight-forward surgery during which the surgeon may discover a tumor or another internal condition. With an instrument according to the invention, the physician can spend a small amount of additional time with the patient under anesthesia and determine the nature and extent of the tumor. This can be particularly beneficial during major surgery, where extending surgery duration poses a potential morbidity and mortality risk. Because the procedure is rapid and noninvasive, the patient is exposed to little additional risk. The benefit of immediate diagnosis and evaluation is significant.

An instrument according to the invention may also be able to provide a wide variety of diagnostic capabilities, allowing a physician to enhance the capabilities of his or her practice substantially in a variety of different realms, without investing in a number of instruments. The

physician can then enhance or update the instrument by the adding software modules that are specifically targeted towards certain conditions of particular tissues, subsystems, or disease states. This can allow a single base instrument to be configured for a variety of different types of practices, and priced according to the type of practice to be served by the instrument. For example, a general-purpose instrument to be used by a general surgeon could include a package of diagnostic protocols that would permit the diagnosis of a variety of conditions that a general surgeon might encounter, while a neurosurgeon's module might be added to allow a specialist to detect particular conditions within the brain. Electronic and optical upgrades may also be provided to update, specialize, or improve the performance of the instrument. Such upgrades can include processing modules, memory boards, lenses, and the like.

Brief Description of the Drawings

Fig. 1 is a perspective diagram of a macroscopic instrument according to the invention;

Fig. 2 is a perspective diagram of a rigid or flexible probe-based instrument according to the invention;

Fig. 3 is a block diagram of the instrument of Fig. 1; and

Fig. 4 is a flowchart illustrating the operation of the system of Fig. 1.

Detailed Description of an Illustrative Embodiment

Referring to Fig. 1, an instrument according to the invention 10 includes an imaging module 12 mounted on a surgical stand 14. In this embodiment, the surgeon can direct the imaging portion 12 towards a patient 20 by manipulating a control 16 that adjusts the attitude of the imaging portion through a positioning mechanism 18.

Referring to Fig. 2, an alternative embodiment of the invention 22 may include a probe such as a rigid or flexible endoscopic, thoracoscopic, laproscopic, or angioscopic probe 24 connected to an imaging station 30 via a fiber-optic cable 26. The surgeon can manipulate the probe within the patient in a minimally-invasive surgical procedure and derive images from a

portion of the patient and display these images on a display 28. A medical implement 32, such as a laser, can also be provided through the probe. For example, after diagnosing a particular condition, a physician can begin laser ablation therapy to remedy it.

Referring to Fig. 3, a medical instrument according to the invention 34 may include an optical acquisition system 36 and a diagnostic processor 38. The acquisition system 36 includes a first-stage imaging optic 40, a Liquid Crystal Tunable Filter (LCTF) 42, a second-stage optic 44, and an imaging element 46. The first-stage optic receives light collected from the patient and focuses it onto the surface of the LCTF. The first-stage optic can be a simple or compound macro lens in the case of a macroscopic instrument (Fig. 1). In a probe-based instrument (Fig. 2), the first stage optic can include imaging optics within a probe such as a endoscopic, laproscopic, thoracoscopic, or angioscopic probe. The first stage lens can also be adjustable, allowing a physician to scan larger areas of tissue and then zoom into particular regions.

The LCTF 42 is a programmable filter that filters out all but a wavelength region of interest from the light collected from the patient. The second-stage optic 44 receives the remaining light from the LCTF and focuses it onto the image sensor 46. The image sensor is preferably, although not necessarily, a two-dimensional array sensor, such as a charge-coupled device array (CCD), which delivers an image signal to the diagnostic processor 38.

The diagnostic processor 38 includes an image acquisition interface 50, that has an input responsive to an output of the image sensor 46 and an output provided to a general-purpose operating module 54. The general-purpose operating module includes routines that perform image processing, and that operate and control the various parts of the system. It has a control output provided to a filter control interface 52, which in turn has an output provided to the LCTF 42. The general-purpose operating module also interacts with a number of diagnostic protocol modules 56A, 56B, ... 54N, and has an output provided to the video display 12. The diagnostic processor can include special purpose hardware, general-purpose hardware with special-purpose software, or a combination of the two. The diagnostic processor also includes an input device 58, which is operatively connected to the general-purpose operating module. A storage device 60, and a printer are also operatively connected to the general-purpose operating module.

In operation, referring to Figs. 3 and 4, a surgeon employing the instrument begins by selecting a diagnostic protocol module using the instrument's input device (step 100). Each diagnostic protocol module is adapted to detect particular characteristics of the surface of one or more types of tissue. For example, the surgeon might select a module which enhances the visibility of cancerous tissue. The surgeon would then direct the camera at the area of interest and begin inspecting it either under ambient light or with the aid of a supplemental light source, which can be filtered to emphasize particular special characteristics of the light it emits.

The diagnostic processor 38 responds to the surgeon's input by obtaining a series of filter transfer functions and an image processing protocol from the selected diagnostic protocol module 56. The diagnostic processor provides the filtering transfer functions to the LCTF 42 via its filter control interface 52 (step 102) and then instructs the image acquisition interface 50 to acquire and store the resulting filtered image from the image sensor 46 (step 104). The general-purpose operating module 54 repeats these filtering and acquiring steps one or more times, depending on the number of filter transfer functions stored in the selected diagnostic protocol module (see step 106). The filtering transfer functions can represent bandpass, multiple bandpass, or other filter characteristics.

Once the image acquisition interface 50 has stored images for all of the image planes specified by the diagnostic protocol chosen by the surgeon, it begins processing these image planes based on the image processing protocol from the selected diagnostic protocol module 56N (step 108). Processing operations can include general image processing of combined images, such as comparing the relative amplitude of the collected light at different wavelengths, adding amplitudes of the collected light at different wavelengths, or computing other combinations of signals corresponding to the acquired planes. The processing operations can also include more complex multivariate statistical techniques to compute the image (e.g., chemometrics). The computed image is displayed on the display 12. It can also be stored in the storage device 60 or printed out on the printer 62.

The processing operations can also be based on a diagnostic knowledge base. This database can include data resulting from the comparison between optical and actual diagnoses.

Each instrument can also continuously update its database as it is used to perform diagnoses, thereby steadily expanding its diagnostic capabilities.

In order to provide a real-time or near-real-time image to the surgeon, the instrument repeatedly acquires planes and processes them to develop an image to be displayed to the surgeon. This allows the surgeon to move the instrument, or to view moving organs, such as a beating heart. This constant acquisition and processing continues until the surgeon either turns the instrument off (step 110) or selects a different imaging mode (step 112). The diagnostic processor 38 preferably has sufficient processing power to update the screen in this way at video rates (i.e., about 30 frames per second), although rates as low as a few frames per second may work quite well, and rates as low as one frame per minute may be adequate for many purposes. On slower instruments, general lock-in schemes or other tracking modalities, such as cardiac gating, can be used to remove motion artifacts due to breathing or heart beat. Frame rate may also be variable, depending on the number of wavelengths and the complexity of the diagnostic procedure.

Preferably, the instrument can operate in multispectral, and hyperspectral, or even ultraspectral imaging modes. Multispectral modes involve image processing derived from a relatively small number of spectral image planes (two wavelengths to about twenty wavelengths). Hyperspectral and ultra spectral imaging modes involve at least twenty image planes and can produce significantly more accurate and informative results. Ultraspectral modes involve hundreds of wavelengths, and may be able to produce even further information about the patient. Hyperspectral and ultraspectral imaging may include selecting specific wavelength bands for discrimination of a particular diseased states, or it may also allow the instrument to scan for multiple conditions at the same time.

It is also contemplated that both types of instrument can operate in connection with an excitation source, such as an ultraviolet lamp and IR source, or other means of spectral illumination or a laser to enhance the received images. Although such excitation may not be necessary, it may allow for the examination of different optical phenomenon and provide additional diagnostic information. And both emission and reflectance modes can be combined in

a diagnostic procedure either simultaneously or sequentially. Relative utilization of different emission or reflection measurements involved in the same diagnostic procedure can be obtained by modulating the different sources. The instrument can also develop light from bioluminescent sources introduced into the patient.

Instruments according to the invention can also operate to process images from image planes acquired at wavelengths outside of the visible region. In one particular embodiment, the instrument is sensitive to the visible and near infra-red regions. It is also contemplated that far infra-red be included to allow the instrument to sense molecular-specific rotational modes.

An example of operation would include the use of a diagnostic protocol module that examined a first wavelength of about 550 and a second wavelength of about 575 associated with oxy- and deoxy-hemoglobin to determine blood oxygenation. The relationship between these wavelengths is described in "Hemoglobin: Molecular Genetics and Clinical Aspects," by H. Franklin Bunn and Bernard Forget, W. B. Sanders, 1986. Another example would include the use of a diagnostic protocol module for examining the Fourier transform infra-red spectra of the colon and rectum as described in "Human Colorectal Cancers Display Abnormal Fourier Transform Spectra," by Basil Rigas et al., Proceedings of the National Academy of Science, pp. 8140-8144, 1987.

Surgical and medical applications of instruments according to the invention can include, but are not limited to, determining tissue viability (i.e. whether tissue is dead or living tissue and whether it is predicted to remain living), detecting tissue ischemia (e.g., in heart, or in leg after a gunshot wound, differentiating between normal and malignant cells and tissues (e.g., delineating tumors, dysplasias and precaucerosus tissue, detecting metastasis), differentiating between of infected and normal (but inflamed) tissue (e.g., extent of aortic root infection), quantification and identification of pathogens, (e.g., bacterial count of burn wounds and differentiating and delineating other pathologic states. Application can also include tissue, blood chemistry, and blood flow (including oxy- and deoxyhemoglobin, myoglobin deoxymyoglobin, cytochrome, pH, glucose, calcium and other elements or biological compounds alone or in combination). The

instrument can also be applied by veterinarians to animals and by dentists to dental applications, such as periodontal disease.

The present invention has now been described in connection with a number of specific embodiments thereof. However, numerous modifications which are contemplated as falling within the scope of the present invention should now be apparent to those skilled in the art. Therefore, it is intended that the scope of the present invention be limited only by the scope of the claims appended hereto. In addition, the order of presentation of the claims should not be construed to limit the scope of any particular term in the claims.

What is claimed is:

1. A medical instrument, including:
 - a first-stage optic responsive to a tissue surface of a patient,
 - a spectral separator optically responsive to the first stage optic and having a control input,
 - an imaging sensor optically responsive to the spectral separator and having an image data output, and
 - a diagnostic processor having an image acquisition interface with an input responsive to the imaging sensor and a filter control interface having a control output provided to the control input of the spectral separator.
2. The medical instrument of claim 1, wherein the spectral separator is a tunable filter.
3. The medical instrument of claim 2, wherein the spectral separator is a liquid crystal tunable filter.
4. The medical instrument of claim 1 wherein the imaging sensor is a two-dimensional imaging array.
5. The medical instrument of claim 1 wherein the imaging sensor includes a charge coupled device.
6. The medical instrument of claim 1 wherein the imaging sensor includes an infra-red sensitive focal plane array.
7. The medical instrument of claim 1 wherein the diagnostic processor includes a general-purpose processing module and a plurality of diagnostic protocol modules.
8. The medical instrument of claim 1 wherein the first-stage optic is a macro lens.
9. The medical instrument of claim 1 wherein the first stage optic is an adjustable lens.

10. The medical instrument of claim 9 further including a stand connected relative to the first-stage optic to position the first-stage optic relative to the patient.

11. The medical instrument of claim 1 wherein the first stage optic includes a probe that includes an imaging fiber optic cable.

12. The medical instrument of claim 1 further including a surgical implement attached to the probe.

13. The medical instrument of claim 1 wherein the control interface is operable to adjust the filter at least twenty times to acquire hyperspectral data for redisplay in real time

14. The medical instrument of claim 1 wherein the diagnostic processor includes a general-purpose processing module and a plurality of diagnostic protocol modules, wherein each of the diagnostic protocol modules includes a plurality of filter transfer functions and an image processing protocol, wherein the general-purpose processing module is operative to instruct the filter to successively apply the filter transfer functions to light collected from the patient, wherein the general-purpose processing module is operative to acquire from the imaging sensor a plurality of images of the collected light each obtained after one of the filter transfer functions is applied, and wherein the general-purpose processing module is operative to process the acquired images according to the image processing protocol to obtain a processed display image.

15. The medical instrument of claim 14 wherein the general-purpose processor is a real-time processor operative to generate a processed display image within a time period on the order of the persistence of human vision.

16. The medical instrument of claim 14 wherein the general-purpose processor is a real-time processor operative to generate a processed display image within about one minute.

17. The medical instrument of claim 16 wherein the general processor is operative to acquire some images more slowly depending on the number of wavelengths and complexity of diagnostic protocols.

18. The medical instrument of claim 1 wherein the diagnostic processor includes a general-purpose processing module and a diagnostic protocol module, wherein the diagnostic protocol module includes a plurality of filter transfer functions and an image processing protocol adapted to detect more than one condition, wherein the general-purpose processing module is operative to instruct the filter to successively apply the filter transfer functions to light collected from the patient, wherein the general-purpose processing module is operative to acquire from the imaging sensor a plurality of images of the collected light each obtained after one of the filter transfer functions is applied, and wherein the general-purpose processing module is operative to process the acquired images according to the image processing protocol to obtain a processed display image.

19. The medical instrument of claim 1 wherein the diagnostic processor includes a real-time processor operative to generate a processed display image within a time period on the order of the persistence of human vision.

20. The medical instrument of claim 1 wherein the diagnostic processor is operable to perform diagnostic processing for images acquired from a source that includes visible light.

21. The medical instrument of claim 1 wherein the filter and sensor are operable in the visible and far infra-red regions.

22. The medical instrument of claim 1 wherein the filter and sensor are operable in the ultra-violet, visible, and infra-red regions.

TRADOCS: 1053380.1 (mksk011.doc)

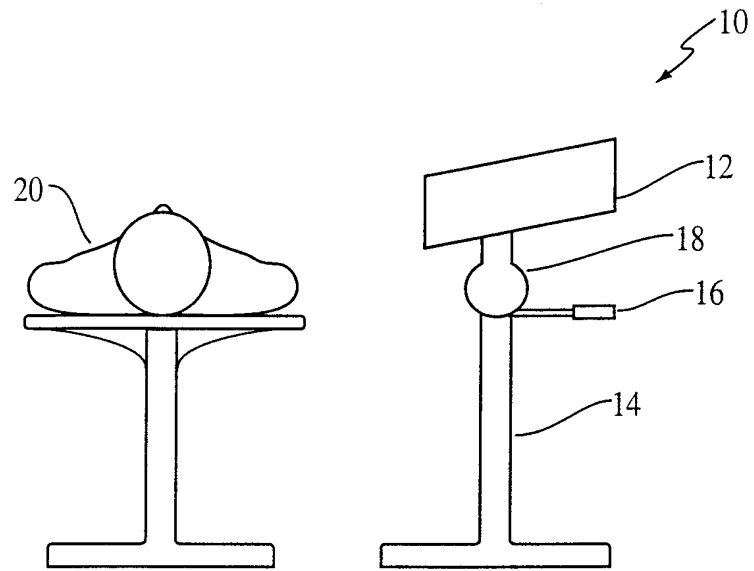


FIG. 1

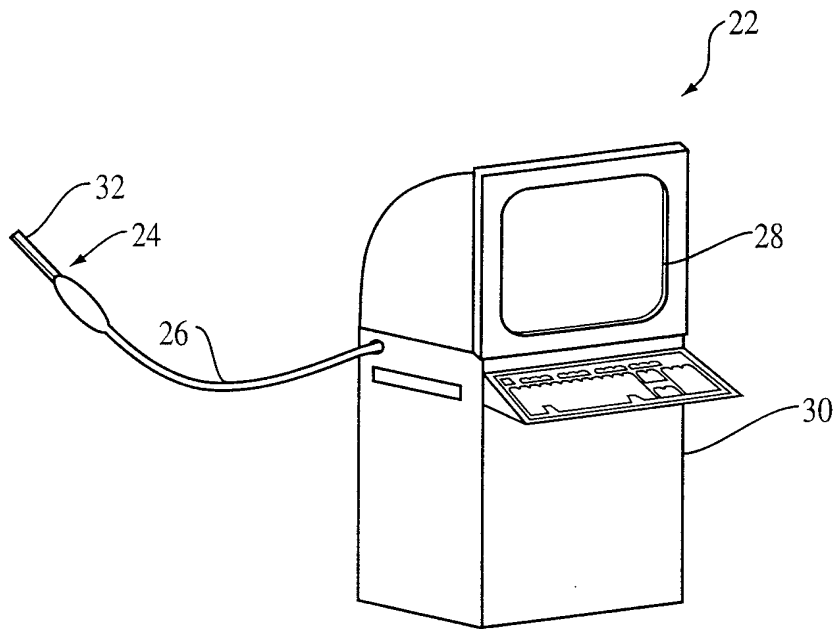


FIG. 2

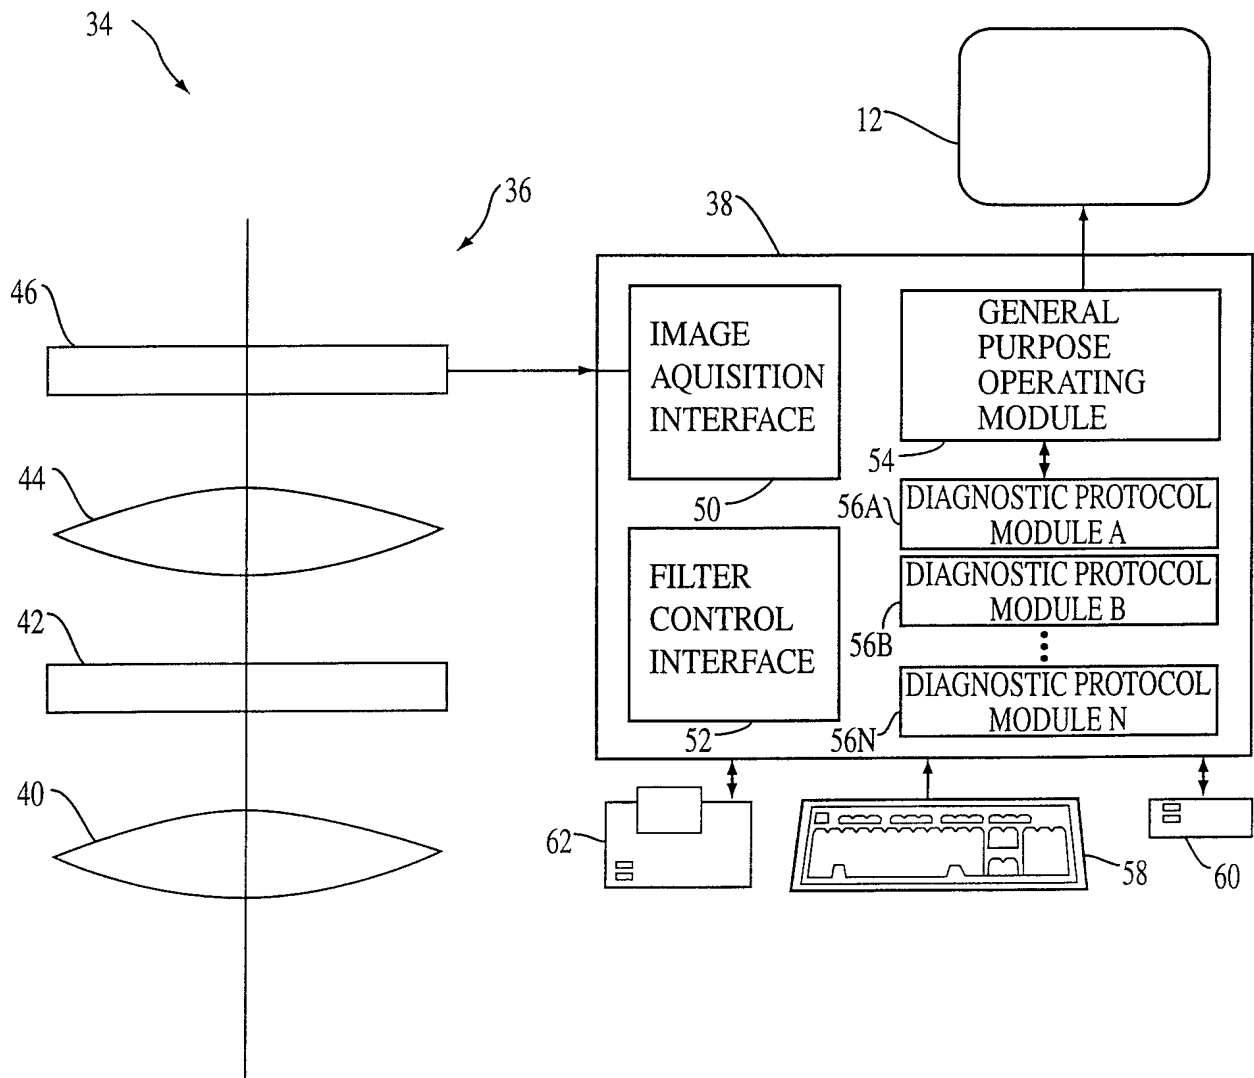


FIG. 3

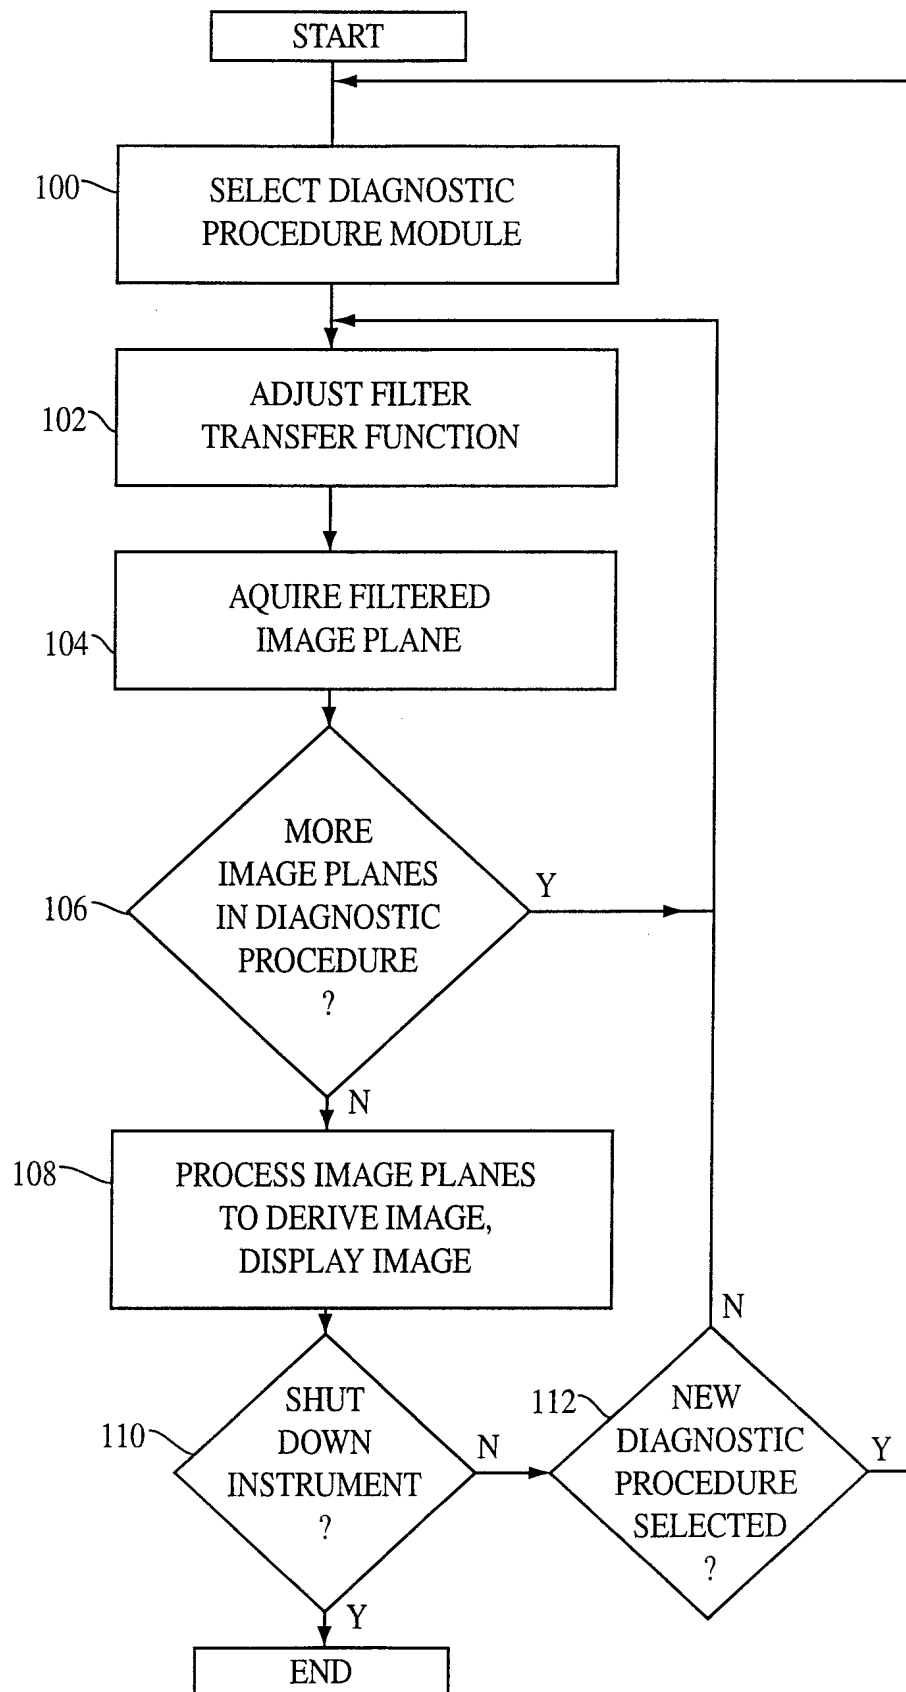



FIG. 4



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁶ : A61B 5/00	A3	(11) International Publication Number: WO 99/22640 (43) International Publication Date: 14 May 1999 (14.05.99)
(21) International Application Number: PCT/US98/22961 (22) International Filing Date: 30 October 1998 (30.10.98) (30) Priority Data: 08/961,294 30 October 1997 (30.10.97) US 60/093,041 10 November 1997 (10.11.97) US (71) Applicant: HYPERMED IMAGING, INC. [US/US]; 315 Russett Avenue, Chestnut Hill, MA 02115 (US). (72) Inventors: LEWIS, Edgar, N.; 18420 Shady View Lane, Brookeville, MD 20833 (US). FREEMAN, Jenny, E.; 27 Lyon Road, Chestnut Hill, MA 02167 (US). (74) Agents: REMENICK, James et al.; Baker & Botts, L.L.P., The Warner, Suite 1300, 1299 Pennsylvania Avenue, N.W., Washington, DC 20004-2400 (US).		(81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GE, GH, GM, HR, HU, ID, IL, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG). Published <i>With international search report.</i> <i>Before the expiration of the time limit for amending the claims</i> <i>and to be republished in the event of the receipt of amendments.</i> (88) Date of publication of the international search report: 19 August 1999 (19.08.99)

(54) Title: MULTISPECTRAL/HYPERSPECTRAL MEDICAL INSTRUMENT

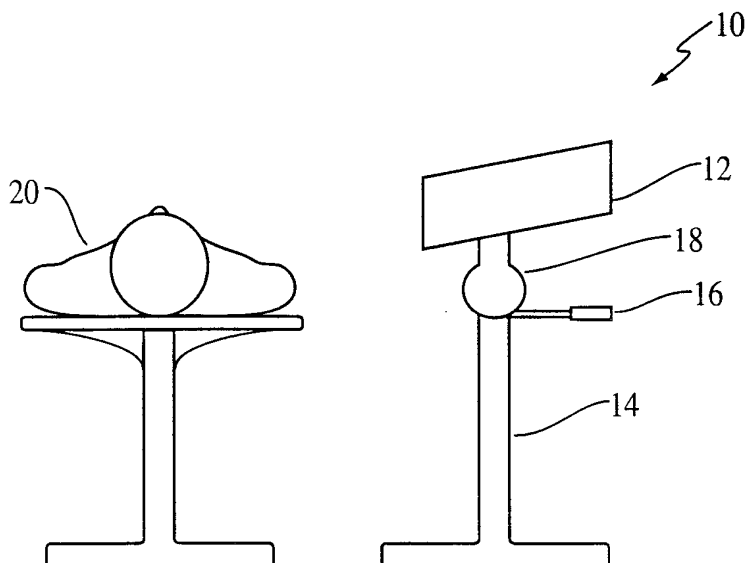**(57) Abstract**

A medical instrument that comprises: a first-stage optic (40) responsive to a tissue surface of a patient; a spectral separator (42) optically responsive to the first stage optic and having a control input; an imaging sensor (46) optically responsive to the spectral separator and having an image data output; and a diagnostic processor (38) having an image acquisition interface (50) with an input responsive to the imaging sensor and a filter control interface (52) having a control output provided to the control input of the spectral separator (42).

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece			TR	Turkey
BG	Bulgaria	HU	Hungary	ML	Mali	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MN	Mongolia	UA	Ukraine
BR	Brazil	IL	Israel	MR	Mauritania	UG	Uganda
BY	Belarus	IS	Iceland	MW	Malawi	US	United States of America
CA	Canada	IT	Italy	MX	Mexico	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NE	Niger	VN	Viet Nam
CG	Congo	KE	Kenya	NL	Netherlands	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NO	Norway	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	NZ	New Zealand		
CM	Cameroon			PL	Poland		
CN	China	KR	Republic of Korea	PT	Portugal		
CU	Cuba	KZ	Kazakstan	RO	Romania		
CZ	Czech Republic	LC	Saint Lucia	RU	Russian Federation		
DE	Germany	LI	Liechtenstein	SD	Sudan		
DK	Denmark	LK	Sri Lanka	SE	Sweden		
EE	Estonia	LR	Liberia	SG	Singapore		

INTERNATIONAL SEARCH REPORT

Inter. Appl. No.

PCT/US 98/22961

A. CLASSIFICATION OF SUBJECT MATTER

IPC 6 A61B5/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 6 A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 96 07889 A (LOCKHEED MARTIN ENERGY SYSTEMS, INC.) 14 March 1996	1-6, 8-11, 20-22
A	see page 4, line 7 - line 28 see page 9, line 5 - page 14, line 17 ---	7,14,18
X	WO 92 15008 A (MASSACHUSETTS INSTITUTE OF TECHNOLOGY) 3 September 1992	1,4-6,8, 9,11,12
Y	see page 3, line 20 - page 7, line 15 see page 11, line 9 - page 14, line 23 ---	2,3,13, 15,16,19
Y	EP 0 783 867 A (UNILEVER PLC ET AL) 16 July 1997	2,3
A	see column 4, line 13 - column 6, line 18 see column 9, line 49 - column 10, line 49 ---	1,4-22
	-/--	



Further documents are listed in the continuation of box C.



Patent family members are listed in annex.

* Special categories of cited documents:

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier document but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- "&" document member of the same patent family

Date of the actual completion of the international search

28 June 1999

Date of mailing of the international search report

06/07/1999

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Geffen, N

INTERNATIONAL SEARCH REPORT

Inter. Patent Application No
PCT/US 98/22961

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	GB 2 300 045 A (Y. PALTIELI) 23 October 1996 see page 1, line 4 - line 12 ----	13,15, 16,19
A	US 4 515 165 A (R. CARROLL) 7 May 1985 see column 3, line 52 - column 5, line 64 ----	1,4-11
A	EP 0 063 431 A (MASAOKI KONOMI) 27 October 1982 see page 5, line 23 - page 7, line 6 -----	1

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 98/22961

Patent document cited in search report		Publication date	Patent family member(s)		Publication date
WO 9607889	A	14-03-1996	US	5599717 A	04-02-1997
			AU	3583395 A	27-03-1996
			BR	9508693 A	06-01-1998
			CA	2230777 A	14-03-1996
			EP	0778939 A	18-06-1997
			NZ	293404 A	25-11-1998
WO 9215008	A	03-09-1992	CA	2104960 A	27-08-1992
			EP	0573535 A	15-12-1993
			JP	6505183 T	16-06-1994
EP 0783867	A	16-07-1997	CA	2186333 A	22-06-1997
			JP	9173048 A	08-07-1997
			US	5760407 A	02-06-1998
GB 2300045	A	23-10-1996	DE	19614374 A	02-01-1997
			FR	2732885 A	18-10-1996
			US	5807264 A	15-09-1998
US 4515165	A	07-05-1985	AU	547510 B	24-10-1985
			AU	6675481 A	13-08-1981
			BE	887366 A	01-06-1981
			CA	1149631 A	12-07-1983
			DE	3103609 A	03-12-1981
			FR	2481454 A	30-10-1981
			GB	2068537 A,B	12-08-1981
			JP	56119232 A	18-09-1981
EP 0063431	A	27-10-1982	JP	57168141 A	16-10-1982
			JP	1513886 C	24-08-1989
			JP	58005631 A	13-01-1983
			JP	63064736 B	13-12-1988
			US	4505583 A	19-03-1985
			DE	3277548 A	03-12-1987